


Instruction for Feline Toxo IgG / IgM Ab test



1 Sampling

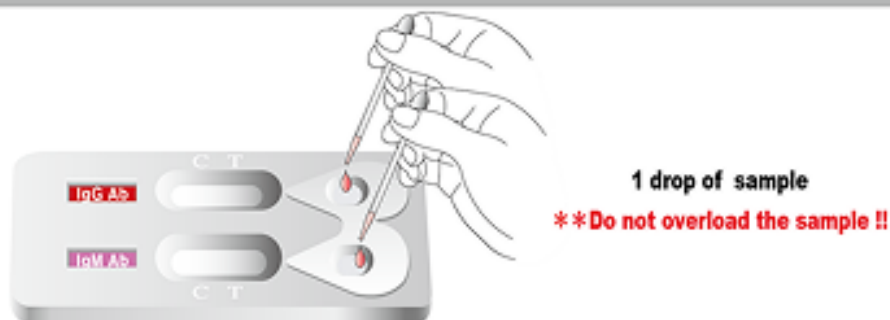


2 Absorption



3 Buffer addition



2 drops of buffer
****after complete absorption**

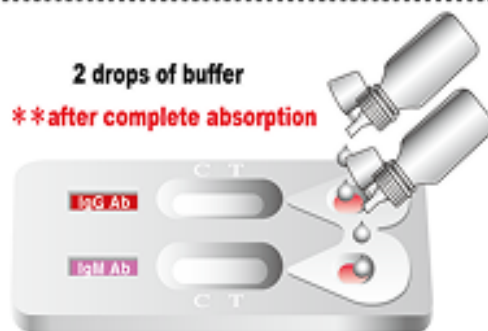

4 Reading

00:05:00 ~ 00:10:00



5 Discard



Discard the used device
In valid result after 10 min

